





1/9

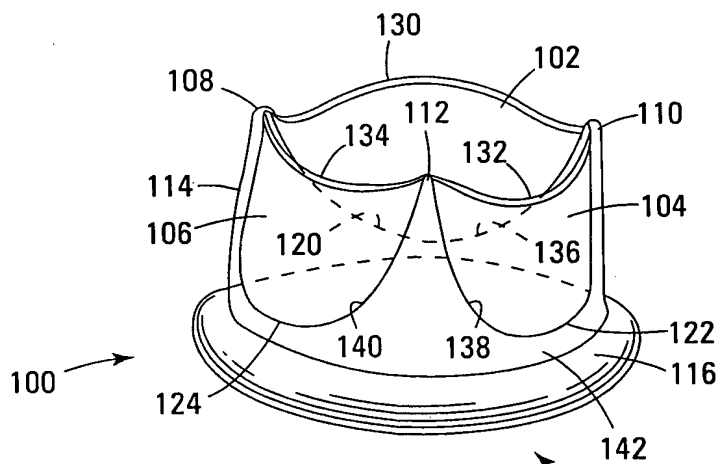

*Fig. 1*

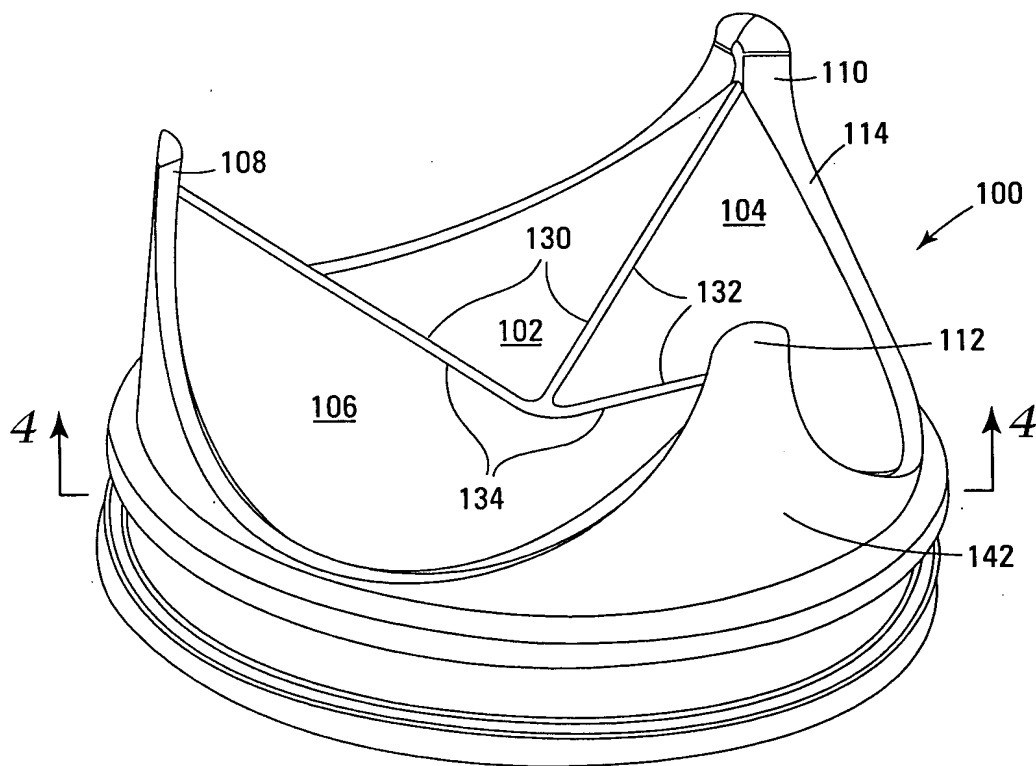


*Fig. 2*

*Fig. 4*




3/9

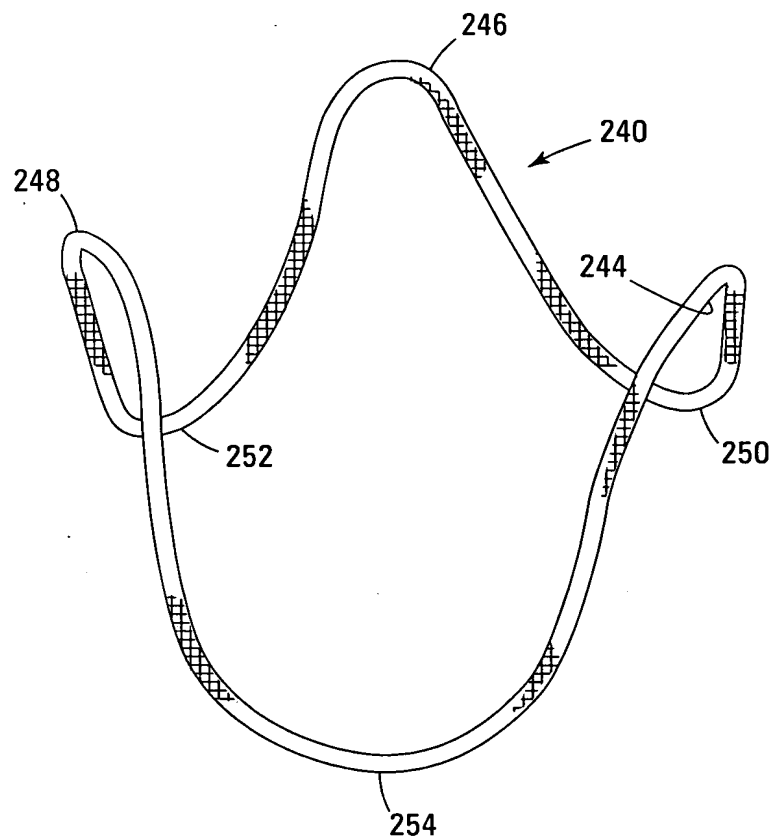

*Fig. 5*



4/9

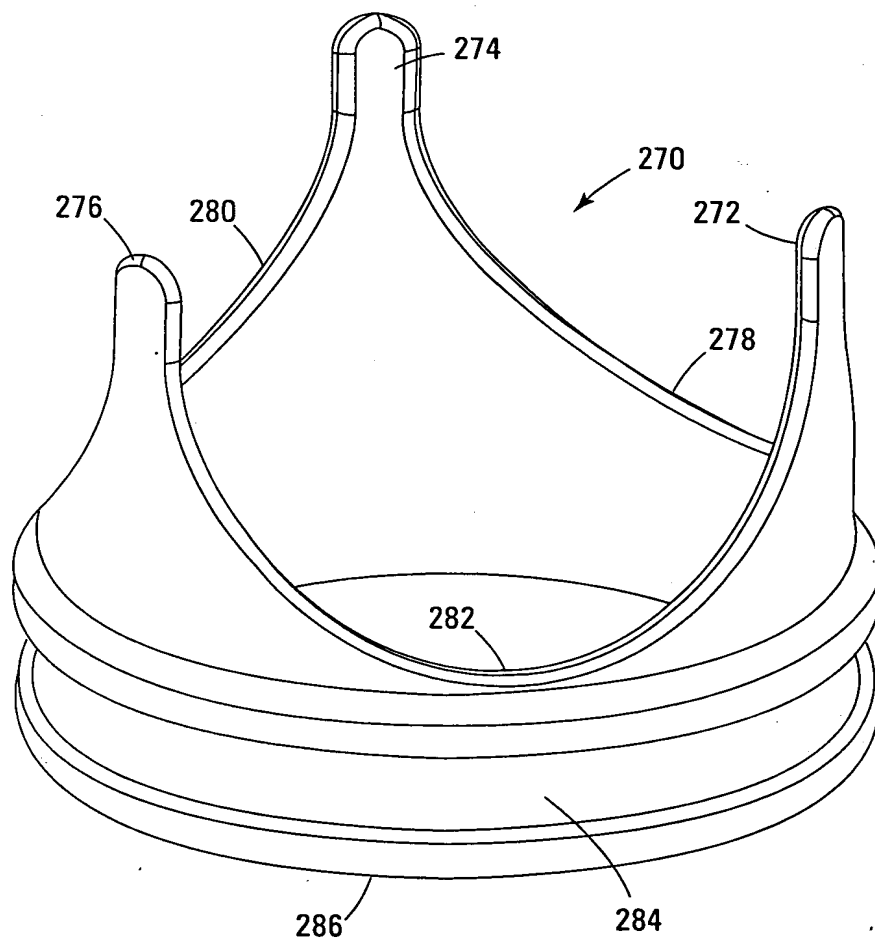

*Fig. 6*


PATENT & TRADEMARK OFFICE

5/9






6/9

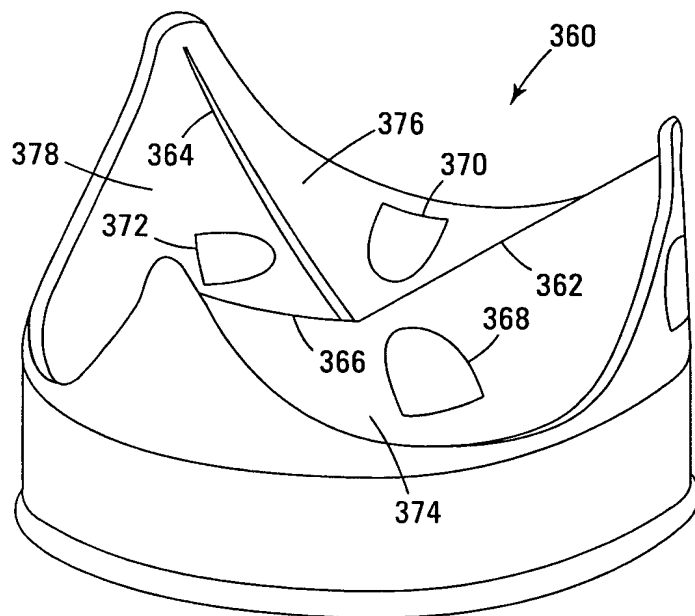

*Fig. 9*

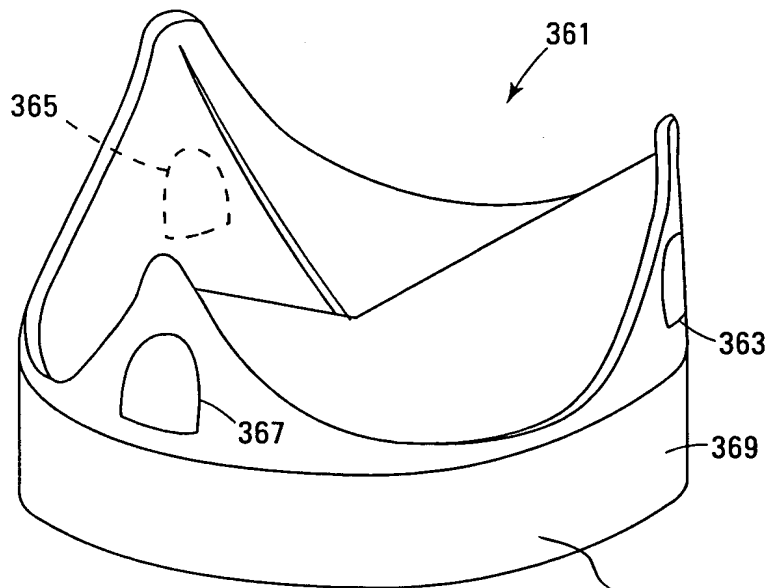


*Fig. 10*



Applicant: Kruse, et al.  
Title: FATIGUE TEST FOR PROSTHETIC STENT  
Atty Docket No. 01610.0108-US-01 Serial No. 10/034,694


7/9

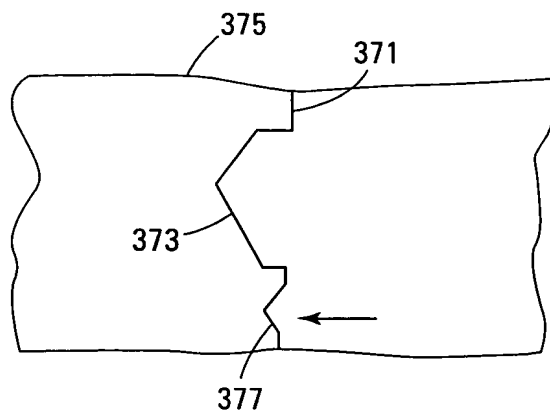


*Fig. 11*



8/9

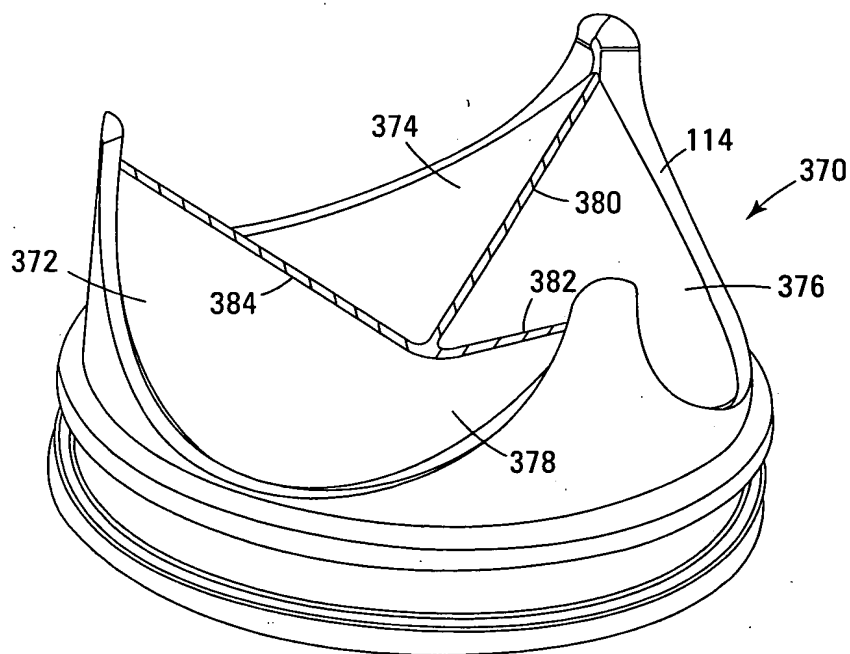

*Fig. 12*

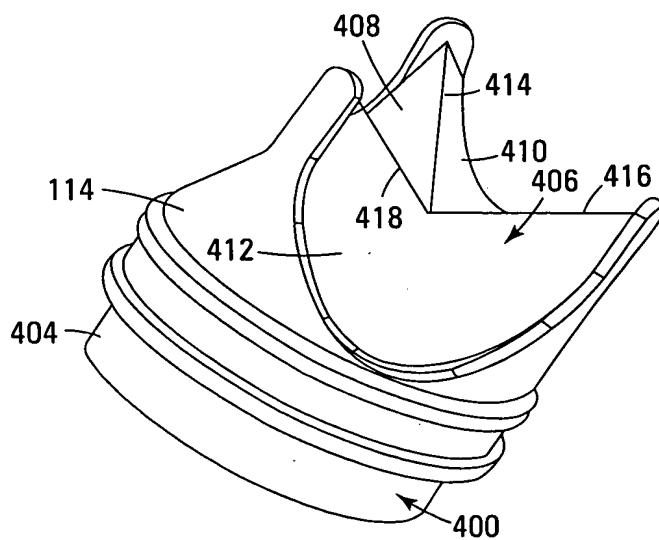


*Fig. 13*






9/9

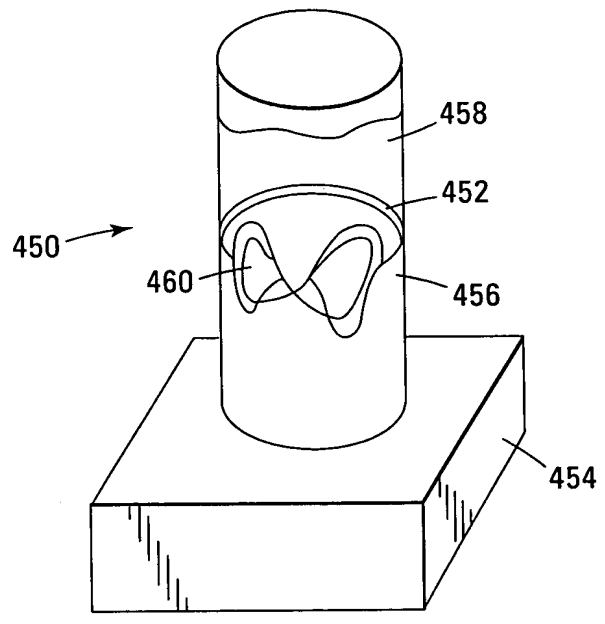

*Fig. 14*

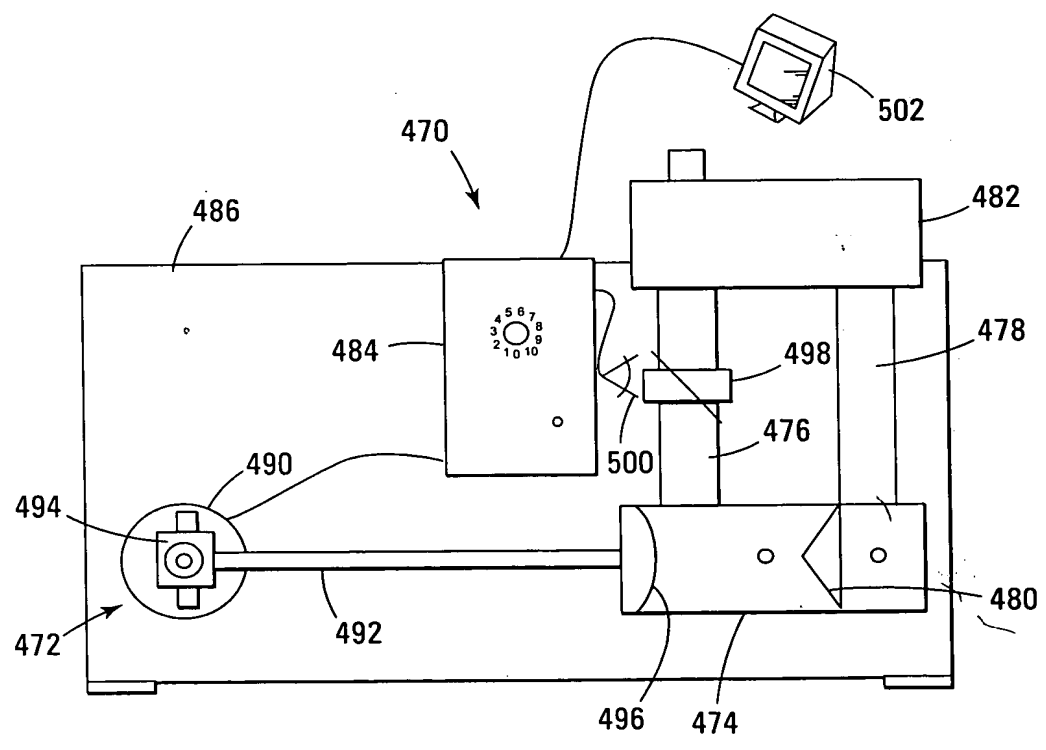

*Fig. 15*